

The Operation Guideline For ONE Step BT Sensor

1. Take out the strips




2. Add milk sample to the micro-well




BALLYA

3. Insert the strips to micro-well


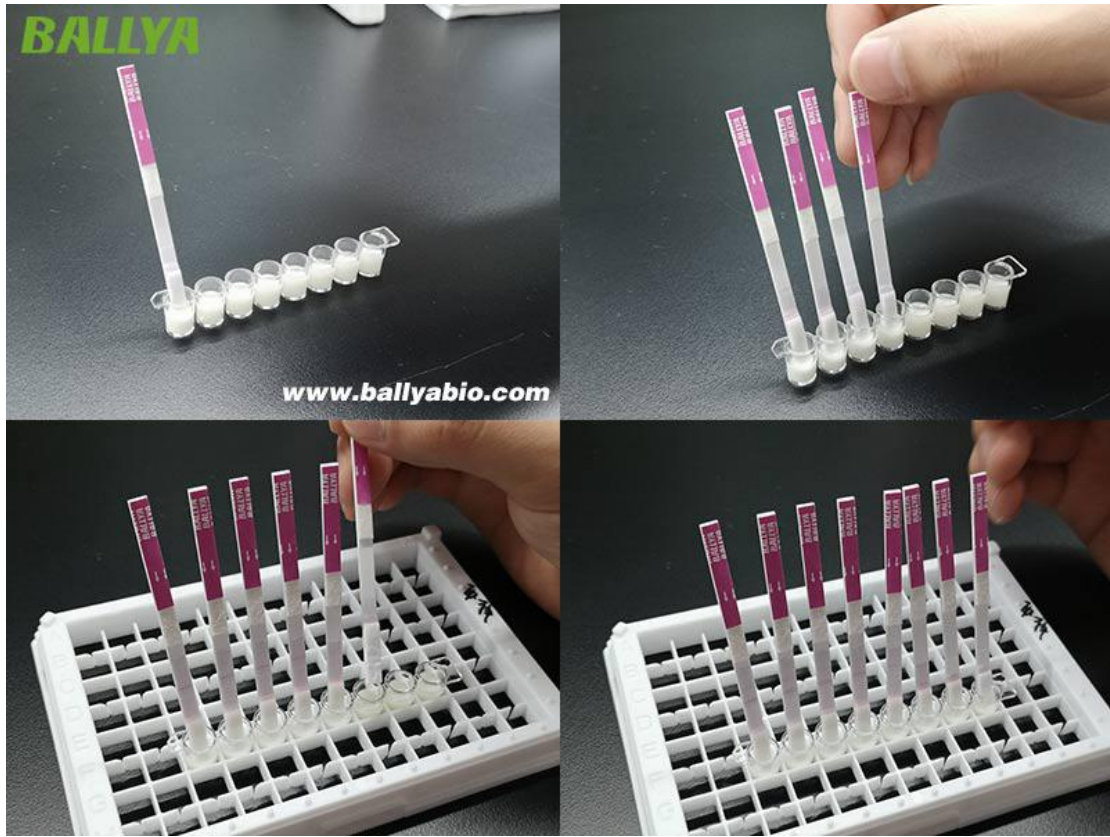


4. Wait for 7 minutes to the results

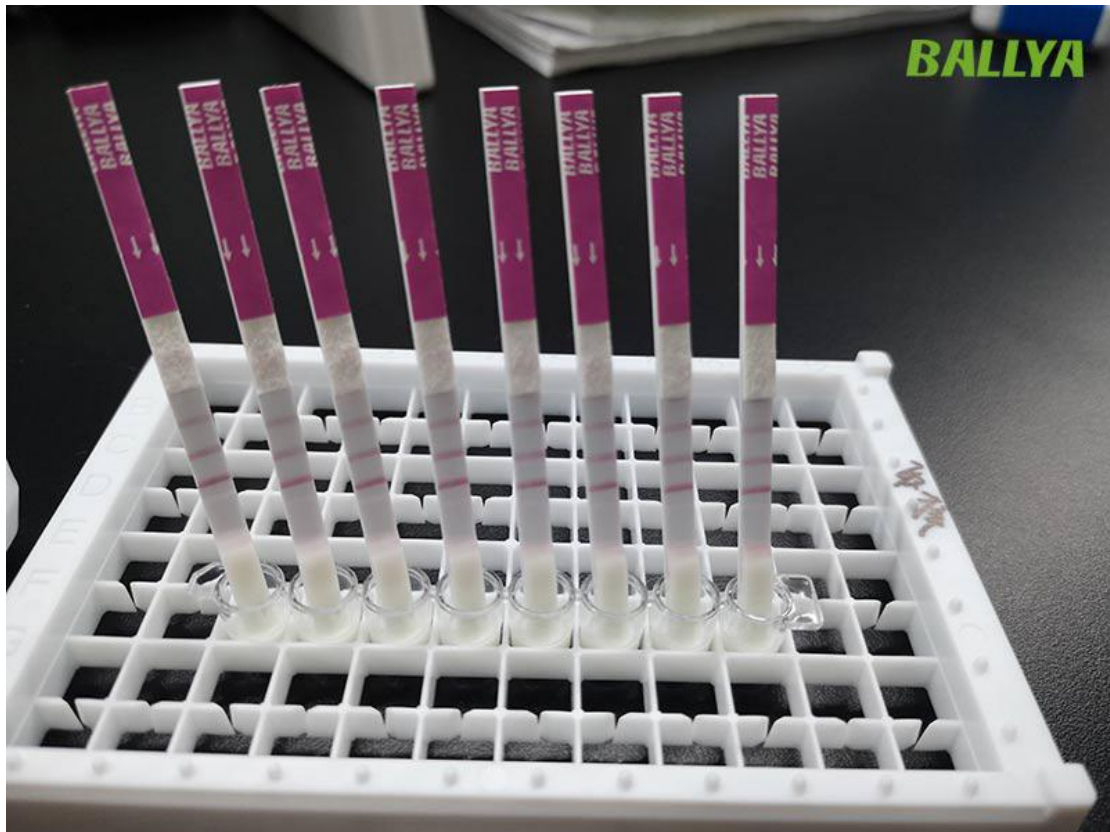

BALLYA

5. Take out the strips and interpret the results

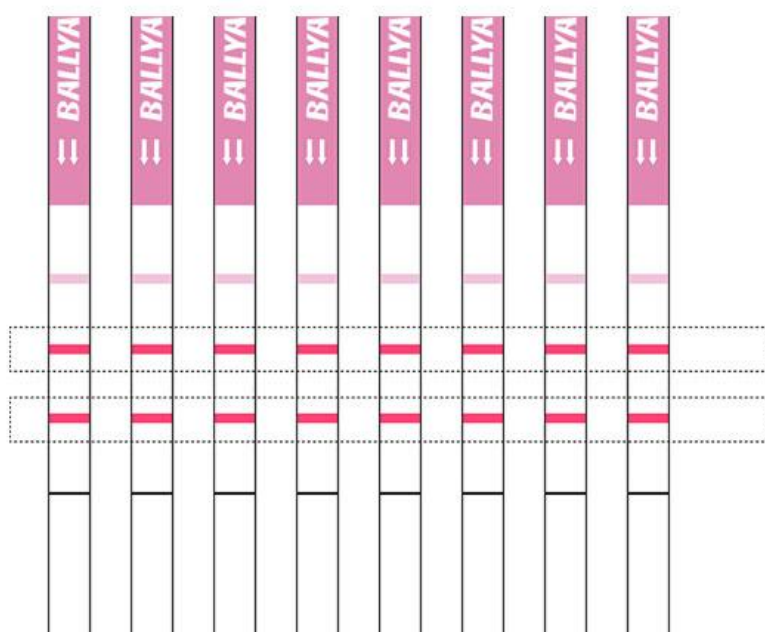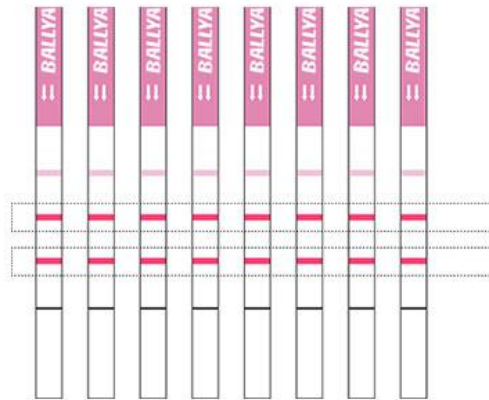

6. Any question, feel free to contact us by email: info@ballybio.com